



OPERATION MANUAL

Series IN 500
IMPAC Pyrometers
IN 510-N • IN 510 • IN 520-N • IN 520



Contents

1	General	5
1.1	Information about the user manual	5
1.1.1	Legend.....	5
1.1.2	Terminology	5
1.2	Safety	5
1.2.1	Electrical connection	5
1.3	Limit of liability and warranty	6
1.4	Unpacking the Instrument	6
1.5	Transport, packaging, storage	6
1.6	Service Request, Repair, or Support	7
1.7	Shipments to LumaSense for Repair	7
1.8	Disposal / decommissioning	8
2	Introduction	9
2.1	Appropriate use	9
2.2	Scope of delivery	9
2.3	Technical Data	9
2.3.1	Dimensions	12
2.4	Components	12
2.5	Accessories (optional)	13
3	Controls and Connections	15
3.1	Installation	15
3.2	Connection cable	16
3.3	Connection	16
3.4	Connecting to serial interface	17
3.5	Sensor head	18
3.5.1	Exchangeability of Sensor heads.....	18
3.6	Exchange of sensor head	19
3.7	Error messages at non-specified sensor temperatures	20
4	Device Settings	21
4.1	Parameters	21
4.1.1	Emissivity (EMI).....	21
4.1.2	Response time (T_{90})	22
4.1.3	Clear time (T_{cl}).....	22
4.1.4	Selection of the maximum or minimum value storage (MAX or MIN)	22
4.1.5	Subrange (LO / HI)	22
4.1.6	Analog output (OUT)	23
4.1.7	Temperature display (°C / °F).....	23
4.1.8	Compensation of ambient temperature (CMP).....	23
4.1.9	Sensor head temperature (AMB).....	23
4.1.10	Baud rate (BD).....	23
4.1.11	Address (AD).....	23
4.1.12	Limit switch (LIM)	23

4.1.13	Hysteresis (HYS).....	24
4.1.14	Wait time.....	24
4.2	Settings at the instrument (only IN 510 and IN 520).....	24
4.3	Settings with HT 6000 (accessory).....	25
5	Software InfraWin.....	27
5.1	Connecting the pyrometer to a PC.....	27
5.2	Installation.....	27
5.3	Program start.....	27
6	Maintenance.....	29
6.1	Safety.....	29
6.2	Service.....	29
7	Data format UPP (Universal Pyrometer Protocol).....	31
8	Reference numbers.....	35
8.1	Reference numbers instruments.....	35
8.2	Reference numbers accessories.....	35
9	Index.....	37

2 Introduction

2.1 Appropriate use

The **IN 510-N, IN 510, IN 520-N, and IN 520** are stationary pyrometers for non-contact temperature measurement of non-metallic surfaces or painted, coated or anodized metals.

The versions IN 510 and IN 520 are equipped with an illuminated LC display which shows the actual temperature reading. All available parameters can be set via the integrated keyboard. The types IN 510-N and IN 520-N do not have display and keyboard, they will be parametrized via the interface.

Type 510 is equipped with a sensor head and sensor cable for an ambient temperature of max. 85 °C without cooling, type 520 is equipped with a sensor head and sensor cable up to 180 °C without cooling.

2.2 Scope of delivery

Instrument, one sensor head with cable length of 3 m or 15 m cable, works certificate, and operation manual.



Note: A connection cable is not included with the instrument and has to be ordered separately (see section **8, Reference numbers**).

2.3 Technical Data

Temperature range:	-40 ... 700 °C (-40 ... 1292 °F)
Sub range:	Factory setting: 0 ... 500 °C; user adjustable (minimum span: 51 °C)
Data handling:	Digital

Spectral range:	8 to 14 µm (for measurement of non-metallic or coated metallic objects)
Sensor head:	Optics 10:1: with lens; optics 2:1: without lens
IR detector:	Thermopile

Power supply:	10 to 30 V DC ripple < 0.5 V power consumption: max. 60 mA
Analog output:	Linear current (0/4 to 20 mA), voltage (0 to 5 V) or thermocouple (type "J" or "K")
Additional output:	10 mV/°C or 10 mV/°F for temperature of sensor head
Load:	Max. 700 Ω / 24 V power supply (for current output) (500 Ω/20 V)
Output impedance:	100 Ω (for thermocouple or voltage output)
Relay contact:	Isolated relay contact; 50 V DC; 0.2 A
Hysteresis:	Negative hysteresis, 2 – 20 °C adjustable (without current or value exceeded = open contact)

Digital interface:	Switchable: RS232 or addressable RS485 (half duplex) baud rate 1200 up to 19200 Bd, resolution 0.1 °C
Isolation:	Non isolated analog outputs and power supply (relay contact isolated)

Emissivity (EMI):	10 to 120% adjustable in steps of 0.1%
Max. / Min. value storage:	Clear time OFF; 0.1 s; 0.25 s; 0.5 s; 1 s; 5 s; 25 s; extern; auto
Response time t_{90} :	180 ms; switchable: 0.5; 1; 2; 5; 10 or 30 s
Temperature display (only IN 510 and IN 520):	LCD, 4 digit, 3 values per second, permanent display illumination
Exceeding of measuring range:	Display: 8888
Fall below measuring range:	Display: 1 °C below sub range
Resolution:	1/10 °C (1/10 °F from -40 to 999.9 °F; 1 °F from 1000 to 1292 °F)

<p>Uncertainty ^{**)}</p> <p>Dependent on object temperature T and ambient temperature T_{amb}. (EMI = 1, t_{90} = 1 s):</p> <p>**) With thermocouple output minimum 2.5 °C</p>	<p>T = 0 to 700 °C: 0.8% or 1 °C ^{*)}</p> <p>T = 0 to -20 °C: 2 °C</p> <p>T = -20 to -40°C: 3°C</p> <p>T_k of uncertainty: 0.03%/°C or 0.05°C/°C at 25 °C ambient temperature T_{amb}. ^{*)}</p> <p>^{*)} Whichever value is greater. The instrument must be at a constant ambient temperature for a minimum of 15 minutes.</p> <p> A correct temperature measurement is impossible if the temperature of the object is more than 85 °C below the sensor head temperature (temperature reading is too high, no error message)</p>
Repeatability:	0.5% of measured value °C or 0.5 °C whichever value is greater, ambient temperature is constant
Noise Equivalent Temperature Difference (NETD):	with t_{90} = 180 ms: 0.1 °C (σ = 1) (measured temperature = 23 °C and emissivity = 1)
Ambient temperature converter:	0 to 65 °C
Storage temperature converter:	-20 to 70 °C
Ambient temperature of sensor head:	IN 510-N and IN 510: 0 to 85 °C IN 520-N and IN 520: 0 to 180 °C with cooling / purging unit: 0 to 200 °C
Storage temperature of sensor head:	-20 to 85 °C (IN 510-N, IN 510) -20 to 180 °C (IN 520-N, IN 520)

Relative humidity:	10 to 95%, non condensing
Protection class:	IP65 (converter, sensor head 10:1, 180 °C-sensor head 2:1) IP20 (85 °C-sensor head 2:1)


Weight:	320 g
Dimensions:	Converter: 98 mm x 64 mm x 34 mm (L x B x H) Sensor head: 28 x 14 mm (L x Ø), thread M12 x 1, L=10.8 mm
Housing:	Aluminum (converter), stainless steel (sensor head)
Operating position:	Any
CE Approval / EMV tests:	According to EU directives about electromagnetic immunity



Note: The calibration / adjustment of the instruments was carried out in accordance with VDI/VDE directive "Temperature measurement in industry, Radiation thermometry, Calibration of radiation thermometers", VDI/VDE 3511, Part 4.4. For additional details on this directive, see <http://info.lumasenseinc.com/calibration> or order the directive from "Beuth Verlag GmbH" in D-10772 Berlin, Germany.


2.3.1 Dimensions

Converter:

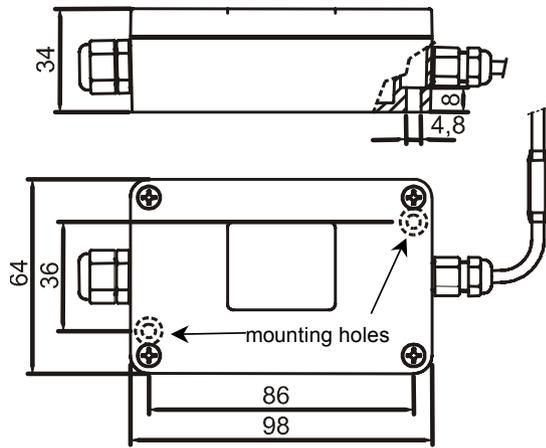


Sensor heads:

Sensor head 10:1

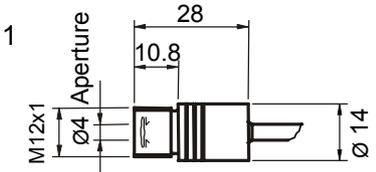


Cable-Ø: approx. 4 mm (types 510)

Sensor head 10:1
with close focus lens



Sensor head 2:1



2.4 Components



Converter



Sensor Head

2.5 Accessories (optional)

Numerous accessories guarantee easy installation of the pyrometers. The following overview shows a selection of suitable accessories. You can find the entire accessory program with all reference numbers on section **8.2 Reference numbers accessories**.



Mounting angle for sensor head



Air purge for sensor head 10:1 and 2:1



*HT 6000:
Portable battery
driven instrument
for setting of
pyrometer
parameters*



*DA 6000:
Led digital display with
possibility for setting of
pyrometer parameters*



*Power supply NG DC
100...240 V AC
⇒ 24 V DC*




*Connecting cable with
additional interface
cable/plug*

3 Controls and Connections

3.1 Installation

The pyrometers are powered by 24 V DC (possible range: 10 to 30 V DC). Ensure correct polarity when connecting the instrument to the power supply. To switch off the instrument, the power supply has to be interrupted.

To meet the electromagnetic requirements (EMV), a shielded connecting cable must be used. The shield of the connecting cable (diameter: 3 - 6.5 mm, max. 12 wires) has to be connected only on the pyrometer's side. If the connecting cable is extended, the shield of the extension also needs to be extended. On side of the power supply (switch board), the shield must be open to avoid ground loops.

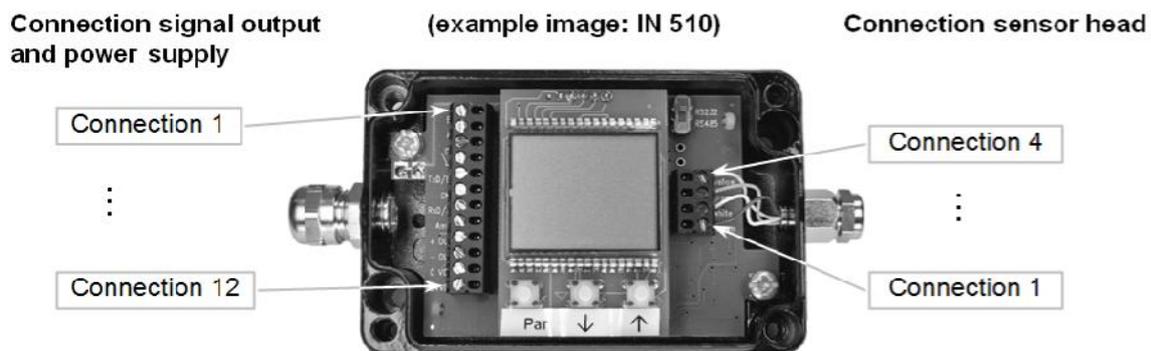

Connection signal output and power supply

1	RS485 „A2“	
2	RS485 „B2“	
3	Relay contact (isolated)	(pink)
4	Relay contact (isolated)	(grey)
5	RS232 interface TxD (RS485 „A1“)	(violet)
6	RS232 interface DGND	(red)
7	RS232 interface RxD (RS485 „B1“)	(black)
8	Sensor head temp. (connection to GND)	(blue)
9	Analog output mA or V or type K or type J (connection to GND)	(green)
10	GND (- OUT)	(yellow)
11	0 V	(brown)
12	+10 ... +30 V DC	(white)

Connection sensor head

4	NTC resistor	(yellow)
3	NTC resistor	(green)
2	Thermopile (+)	(white)
1	Thermopile (-)	(brown)

Note:

- The sensor head is already connected to the converter (state of delivery).

3.2 Connection cable


The connecting cable has to be selected according to the following criteria:

- Shielded
- Diameter 3 - 6.5 mm
- Number of wires: 2 to 12 (as required)
 - 2 for power supply.

additionally, if required:

- 1 for analog output
- 1 for sensor head temperature
- 1 GND for analogue output and / or sensor head temperature
- 3 or 4 for digital interface
- 2 for relay contact

Fig. 1

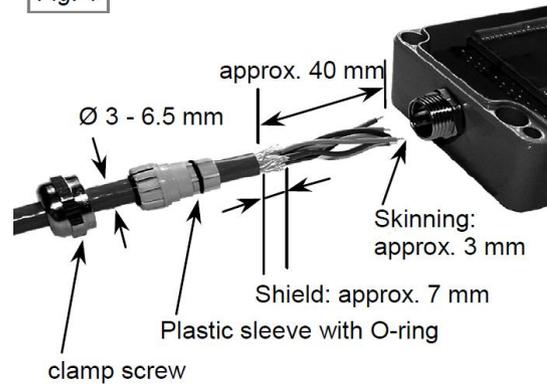


3.3 Connection

1. Prepare the cable as shown in Fig. 1.
2. The shielding of the connecting cable has to be pushed over the plastic sleeve 2 mm further than the O-ring.
3. Fix the cable with the clamp screw.
4. At state of delivery, an internal connection between contact 11 and the housing exists. Should the housing have its own earth potential caused by an electric connection to an object, the internal connection has to be removed. Fig. 2.

The screw bars inside the converter can be lifted up for easy installation of the wires (input/output cables and sensor head) Fig. 3.

Grounding Wire Bridge

Fig. 2

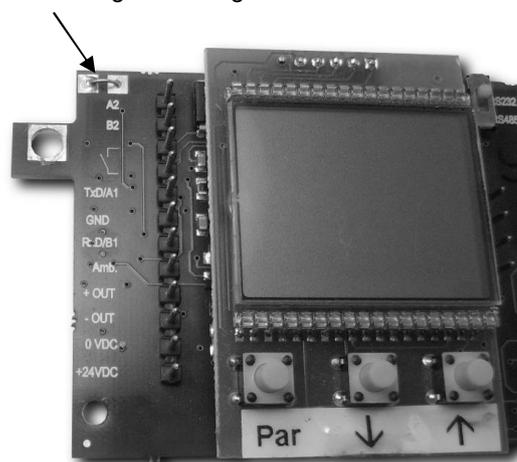

Caution: Before connecting the pyrometer to other instruments (e.g. controller, PLC, etc.), the correct analog output (current, voltage or thermocouple) corresponding to the input of the instrument, has to be adjusted at the converter. A wrong output might damage the connected instrument.


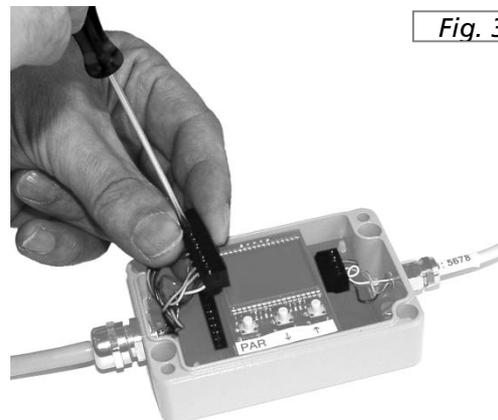


Fig. 3

Fig. 4 : There are two holes with 4 mm screws for mounting the converter housing.

After mounting, connecting cables and parametrizing (if necessary), close the cover of the converter and tighten the 4 screws.

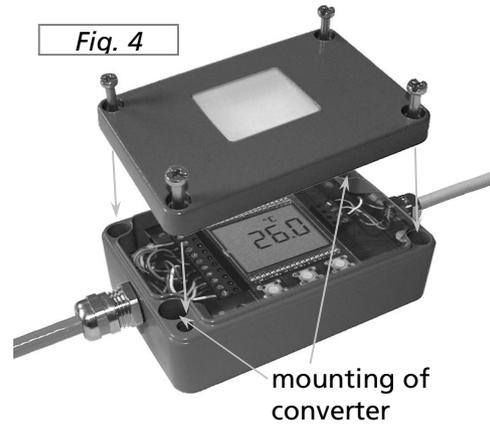

Note: If using the pyrometer with measuring output thermocouple type K or J, this output has to be connected with the correct compensating cable.

3.4 Connecting to serial interface


The pyrometers are equipped with a serial interface RS232 or RS485 (switchable at the pyrometer). Only short distances can be transmitted with RS232 and electromagnetic interferences can affect the transmission. With RS485. The transmission is, to a large extent, free of problems. Long transmission distances can be realized and several pyrometers can be connected in a bus system.

The transmission rate (in baud) of the serial interface is dependent on the length of the cable. Values between 1200 and 19200 Bd may be set.

Typical cable length for RS232 at 19200 Bd is 7 m.

Typical cable length for RS485 at 19200 Bd is 2 km.

Connection example of 2 instruments with RS485:

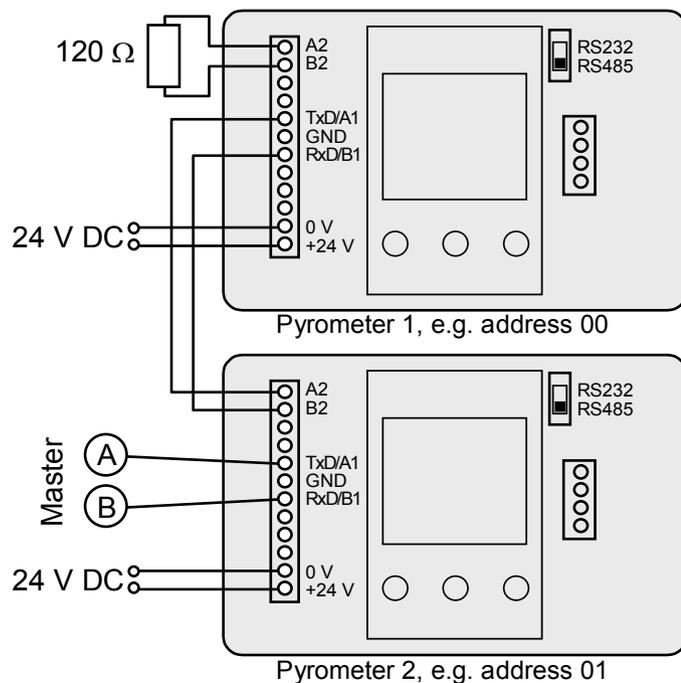

3.5 Sensor head


Two different optical head types with a field of view of 10:1 or 2:1 are available. The spot sizes at different measuring distances are shown in the drawings below; intermediate values have to be interpolated. An additional close focus lens is available for the 10:1 head of series 510 instruments (temperature resistant up to 85 °C). It can be used to generate a small spot size in a short distance.

3.5.1 Exchangeability of Sensor heads

Whether a sensor head can be used with a different electronic box is indicated by the identifier "S1" on the sensor cable:

- IN 500 (legacy product): optical heads 2:1 (S1 0xxx) and 10:1 (S1 1xxx) can be used with any electronic box.
- IN 510: optical heads 2:1 and 10:1 (both S1 0xxx) can be used with any electronic box.
- IN 520: optical heads 2:1 and 10:1 (both S1 2xxx) can only be used with IN 520 electronic boxes

When connecting a new sensor head to the electronic box, the respective 8-digit pin-code has to be set (see section 3.6, **Exchange of sensor head**).

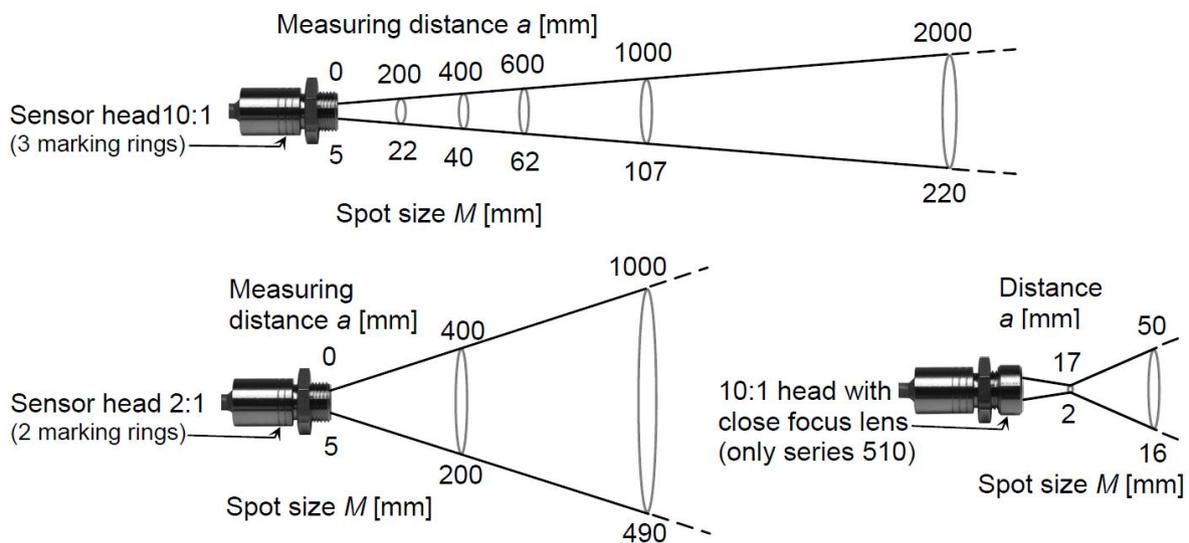

Note: The pyrometer can measure objects at any distance but the farther the distance, the larger is the measuring area (spot size). The object has to be bigger than, or at least as big as the spot size of the pyrometer in the measuring distance.


3.6 Exchange of sensor head

Note: Whether a sensor head can be used with a different electronic box is indicated by the identifier "S1" on the sensor cable. See section 3.5.1 for more information.

The sensor head is exchangeable if a sensor head with other optical data or a longer cable is required. Each sensor head cable is marked with a label containing a sensor code which has to be set in the pyrometer.

The sensor head cable is available in lengths of 3 or 15 m which can be cut to any required length. The sensor code label should be affixed to the remaining part of the cable.

The cable has to be prepared as shown in the illustration. The shield must be pushed above the washer and O-rings, then the cable can be pushed into the converter and fixed with the clamp screw (series 510) or soldered to the pins (series 520). (For cable connection, see schematic in section 3.2, **Connection cable**.)

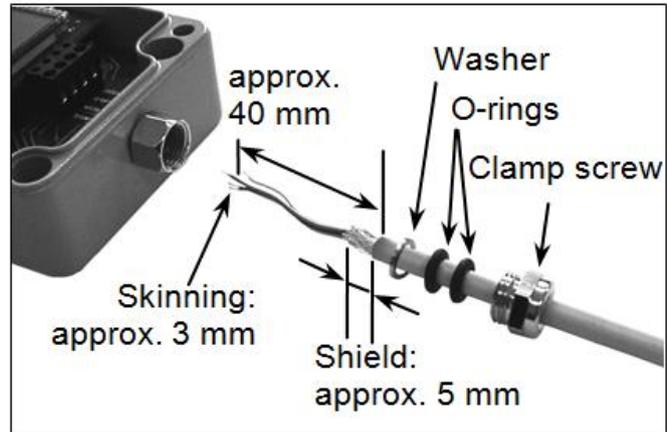

The sensor code at the cable has to be set in the pyrometer as follows:

- Setting via software: Set these codes S1 and S2 in **"Pyrometer parameters"** under the button **Exchange sensor head** and confirm them with **"OK"**. Now the new sensor head is matching to the converter and the pyrometer is ready for measuring.
- Additionally in the IN 510 or IN 520, the setting of the sensor head codes can be done via internal push buttons: Remove the cover of the converter and press the buttons **↑** and **↓** simultaneously. While pressing these two buttons, push the **"PAR"** button too. The display shows code S1. With the arrow buttons **↑** and **↓**, the new code S1 has to be set and confirmed with the **"PAR"** button. Now code S2 appears on the display and has to be set and confirmed in the same way.
- A setting of these codes with the HT 6000 or digital display DA 6000 is not possible.



3.7 Error messages at non-specified sensor temperatures

The pyrometer gives the following error messages for the protection of the electronics and the machines if the temperature of the sensor head is out of specified values:

- Excess of specified sensor head temperature (corresponding to the model: 85 °C or 180 °C):
 - Output of the serial interface code 75550
 - Output of the analog output: 22 mA at 0/4 to 20 mA, 5 V at 0 to 5 V, excess of end of measuring range at thermocouple output
 - The relay is de-energized (contact open)
 - Display of (IN 510 or IN 520): ERR 1 instead of the temperature reading
- Sensor head temperature falls below specified value (0 °C):
 - Output of the serial interface code 74440
 - Output of the analog output: 22 mA at 0/4 to 20 mA, 5 V at 0 to 5 V, excess of end of measuring range at thermocouple output
 - The relay is de-energized (contact open)
 - Display of (IN 510 or IN 520): ERR 2 instead of the temperature reading

There is no error message if the converter temperature runs out of its specified operating temperature.

4 Device Settings

4.1 Parameters

The setting of the parameters of the **IN 510-N or IN 520-N** can only be done via serial interface (see section **4.3 Settings with HT 6000 (accessory)**), the parameters of the **IN 510** and **IN 520** additionally can be done using the integrated push buttons inside the converter (see section **4.2 Settings at the instrument**).

4.1.1 Emissivity (EMI)

For a correct measurement, it is necessary to adjust the emissivity. This *emissivity* is the relationship between the emission of a real object and the emission of a black body radiation source (this is an object which absorbs all incoming rays and has an emissivity of 100%) at the same temperature.

Different materials have different emissivities ranging between 0% and 100% (settings at the pyrometer between 10 and 100%, an additional attenuation, setting from 100 to 120% can be used for example to correct the measurement of objects behind gases with hot soot).

Additionally, the emissivity is dependent upon the surface condition of the material, the spectral range of the pyrometer and the measuring temperature. The emissivity setting of the pyrometer has to be adjusted accordingly.

Typical emissivity values of various common materials for the spectral range of the instruments are listed below. The tolerance of the emissivity values for each material is mainly dependent on the surface conditions. Rough surfaces have higher emissivities.

Object	Emissivity (%)
" Black body furnace "	100
Human skin	98
Black dull varnish	95
Carbon soot	95
Wood	80 ... 92
Paper	92 ... 95
Asphalt	85
Glass / Quartz glass	72 ... 87
Textile	75 ... 95
Graphite	75 ... 92
Cement	90
Water	95

Object	Emissivity (%)	
Brickwork	}	
Fire clay		
Rubber		
Porcelain		85 ... 95
Ceramics	}	
Varnish		
Plaster		
Oil paint		
Steel (oxidized)	60 ... 80	
Steel (smooth)	10 ... 30	
Aluminum (smooth)	2 ... 15	
Aluminum (anodized)	96	

4.1.2 Response time (T_{90})

The response time t_{90} is the time interval for the analog output of the pyrometer to go from a low temperature value up to 90% of the temperature step to a high value when measuring an abrupt increase from said low to said high temperature. The time is taken to reach 90% of the recorded temperature difference. In the OFF position, the device operates using this time constant (shortest response time).

Longer response times can be used for the measurement of objects which have rapidly fluctuating temperatures to achieve constant temperature reading.

Settings:
OFF
0.5 s
⋮
30 s

4.1.3 Clear time (T_{cl})

The *maximum value storage* (or minimum value storage) stores the highest (or lowest) measurement value. The clear time defines the time period until the stored value is deleted and replaced by a new one.

The following settings are possible:

- When set to OFF, the maximum value storage is switched off and all new temperature values are measured but not stored.
- If any clear time between 0.01 s and 25 s is set, the maximum value is estimated and held in storage mode. After the entered time, the storage will be deleted.
- The "auto" mode is used for discontinuous measuring tasks. For example, objects are transported on a conveyer belt and pass the measuring beam of the pyrometer only for a few seconds. Here the maximum (minimum) value for each object has to be indicated. In this mode, the maximum (minimum) value is stored until a new hot (or cold) object appears in the measuring beam. The temperature which has to be recognized as "hot" (or "cold") is defined by the low (high) limit of the adjusted sub range. The stored maximum value will be deleted when the temperature of the new hot object exceeds the low limit **LO** of the sub range by 1% or at least 2 °C. The stored minimum value will be deleted when the object temperature falls below the high limit **HI** of the sub range by 1% or at least 2 °C.
- The external clearing ("extern") of the storage can only be activated and used with an own software (see data format **UPP**[®], section 7).

Settings:
OFF
0.1 s
⋮
25 s
extern
auto

4.1.4 Selection of the maximum or minimum value storage (MAX or MIN)

With this setting you choose between maximum or minimum value storage if the storage function is activated by setting **TCL**. If **TCL** is switched "OFF", the storage function is not activated, the indication of "MAX" or "MIN" only shows the preselection.

Settings:
MAX
MIN

4.1.5 Subrange (LO / HI)

You have the opportunity to choose a subrange (minimum 51 °C) within the basic measuring range of the pyrometer. This subrange corresponds to the analog output. **LO** describes the beginning of this measuring range, **HI** the end of the range. If the thermocouple output is used, the analog output does not change. In addition, by setting a subrange, it is possible to fulfill the requirements of the "auto" clear mode of the maximum or minimum value storage (see above).

Settings:
700 °C
⋮
-40 °C

4.1.6 Analog output (OUT)

The analog output has to be selected according to the signal input of the connected instrument (controller, PLC, etc.). You can choose between current output (0 or 4 to 20 mA), voltage output (0 to 5 V) or thermocouple output type J or K.

Settings:
0-20 mA
4-20 mA
0-5 V
type J
type K



Caution: Before connecting the pyrometer to other instruments (e.g. controller, PLC, etc.) the correct analog output (current, voltage or thermocouple), corresponding to the input of the instrument, has to be adjusted in the converter. A wrong output might damage the connected instrument.

4.1.7 Temperature display (°C / °F)

The temperature can be displayed in °C or °F.

Settings:
°C
°F

4.1.8 Compensation of ambient temperature (CMP)

This compensation is used for a very few special applications only. The standard setting of this parameter is "auto", because the temperature of the sensor head is normally the ambient temperature of the measured object. Should the measured object be placed in an area with a higher ambient temperature (e.g. inside a furnace), the measurement might be falsified (probably too high temperature indication). This influence can be compensated by presetting of the ambient temperature of the object with help of the CMP-function (presetting within the measuring range of the instrument). It has to be considered, that this method only improves the results if the ambient temperature at the place of the measured object is always constant.

Settings:
700 °C
⋮
-40 °C
auto

4.1.9 Sensor head temperature (AMB)

The temperature of the sensor head can be displayed.

4.1.10 Baud rate (BD)

The transmission rate of the serial interface in Baud (Bd) is dependent on the length of the cable. The standard cable length with RS232 for 19200 Bd is 7 m, with RS485 2 km. The baud rate is reduced by 50% if the transmission distance is doubled.

Settings:
19200 Bd
⋮
1200 Bd

4.1.11 Address (AD)

To connect several pyrometers with RS485 (up to 32) with one serial interface, it is necessary to give each instrument an individual address for communication. First it is necessary to connect each single instrument to give it an address. After that, all instruments can be connected and addressed individually. If parameters may be changed simultaneously on all pyrometers, the global **address 98** can be used. This allows you to program all pyrometers at the same time, regardless of the addresses that have already been assigned. If the address of a pyrometer is unknown, it is possible to communicate with it using the global **address 99** (connect only one pyrometer).

Settings:
31
⋮
00

4.1.12 Limit switch (LIM)

The instruments are equipped with a relay contact, controlled by the measuring signal. The switch point of this relay is adjustable with the function "LIM" within the measuring range. The relay contact is closed below the adjusted value, it is open above it.

Settings:
700 °C
⋮
-40 °C

4.1.13 Hysteresis (HYS)

The relay contact opens immediately when the temperature exceeds the adjusted "LIM" value, it closes only if the temperature falls below a value which consists of "LIM" and the adjusted hysteresis.

Settings:
20°C
⋮
2°C

4.1.14 Wait time

(only available via interface commands, see Chapter 7, Data format UPP)


When using a pyrometer with RS485, it is possible that the connection is not fast enough to receive the pyrometer's answer to an instruction of the master. In this case, a wait time can be set to slow down the data transfer (e.g.: tw = 02 at a baud rate 9600 means a wait time of 2/9600 sec).

Standard settings at delivery:

EMI=100; T90=OFF; TCL=OFF; MAX/MIN=MAX; OUT=0...20 mA; LO=0 °C; HI=500 °C; °C/°F=°C; CMP=auto; BD=19200; AD=00; LIM=0 °C; HYS=2 °C

4.2 Settings at the instrument (only IN 510 and IN 520)

The buttons for parametrizing the IN 510 or IN 520 are inside the converter and are accessible after removing the cover (4 screws).

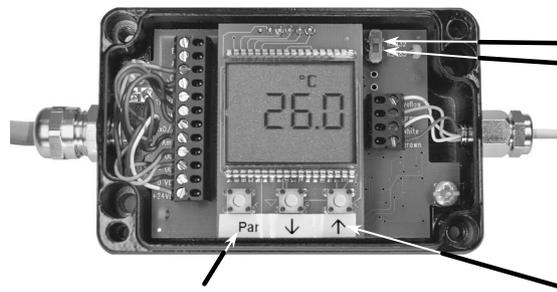

Interface switch:

RS232
RS485

Selection of parameters: the parameters are called with the button **PAR** (the sequence is described on section 4). If no button is pushed for approx. 15 s, the instrument switches back to measuring mode with the latest parameter settings. A changed value of a parameter is automatically stored after changing to another parameter.

Up / down buttons (↑ ↓): After selection of one parameter with the PAR button the up / down buttons are used to set the available values.




Note: Do not operate the converter permanently with open cover.

4.3 Settings with HT 6000 (accessory)

The HT 6000 is a portable battery driven instrument for the parameter setting of digital pyrometers and for indication of temperature.

The pyrometer has to be connected to the HT 6000 via its interface cable (RS232 or RS485) with the female SUB-D connector. When the HT 6000 is switched on, it automatically recognizes the pyrometer and allows the preset parameters to be displayed. With the "PAR" button the different parameters can be called in the sequence described on section **4.1 Parameters**. With the arrow buttons, the values of the parameters can be selected and confirmed with the "ENTER" button. If no button is pressed for 30 s the HT 6000 changes to the temperature indication **without accepting the changed value**.

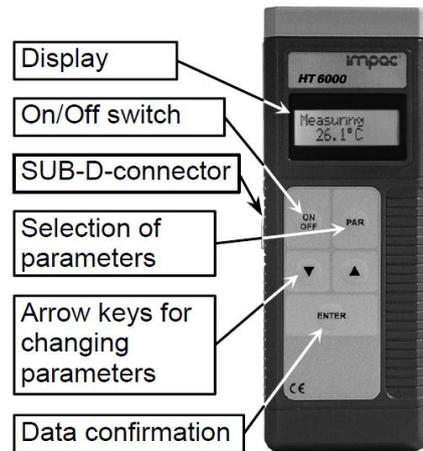

5 Software InfraWin

The operating and analyzing *InfraWin* software is included with delivery of the pyrometer. In addition to allowing you to make parameter adjustments via PC, the *InfraWin* software also provides temperature indication, data logging, and measurement analysis features.

A software description can be found in the program's help menu. Click on the F1 button after loading *InfraWin* or click on the ? in the menu bar.

The latest version is available for free as download from the homepage www.lumasenseinc.com.

5.1 Connecting the pyrometer to a PC

The program *InfraWin* can operate up to two devices. Two devices using RS485 may be operated simultaneously by the same interface, if two different addresses have been properly entered (see section 4.1.11 **Address** for more information).

5.2 Installation

To install the *InfraWin* software, select setup.exe from the *InfraWin*-CD or from the downloaded and unpacked zip file from the internet and then follow the installation instructions.

5.3 Program start

The first time you load *InfraWin* 5, you will be prompted to select a default language. The *InfraWin* software is available in German, English, Spanish, French, Portuguese, and Chinese. Once installed, click **Language/Languages** if you would like to select another language.

6 Maintenance

6.1 Safety

Attention during pyrometer services:

Should the pyrometer be integrated in a running machine process, the machine has to be switched off and secured against restart before servicing the pyrometer.

6.2 Service

The pyrometer does not have any parts which require regular service, only the lens has to be kept clean. The lens can be cleaned with a soft cloth in combination with alcohol (do not use acid solutions or dilution). Also standard cloths for cleaning glasses or photo objectives can be used.

The lens of the 10 : 1 sensor head has an anti-reflective coating which appears slightly colored.



Caution: Be extremely careful - this layer can easily be rubbed off - this will greatly affect the measuring results!

7 Data format UPP (Universal Pyrometer Protocol)

Via interface and suitable communication software or via "Test" function of the *InfraWin* software (section "pyrometer parameters") commands can be exchanged directly with the pyrometer.

The data exchange occurs in ASCII format with the following transmission parameters:

The data format is: 8 data bits, 1 stop bit, even parity (8,1,e)

The device responds with the entry of a command with: output (e.g. the measuring value) + CR (Carriage Return, ASCII 13), with pure entry commands with "ok" + CR. With invalid commands the instruments answers with „no" + CR.

Every command starts with the 2-digit device address AA (e.g. "00"). This is followed by 2 small command letters (e.g. "em" for level of emissivity ϵ), finished with CR

This is followed, if necessary for that command, by the ASCII parameter "X". If this parameter "X" is omitted, then the device resets with the current parameter.

Example: Entry: "00em" + <CR>

The emissivity setting of the device with the address 00 is returned

Answer: "0970" + <CR> means emissivity = 0.970 or 97.0%

Description	Command	Parameters
Reading measuring value:	AAms	Output: YYYYY; 5-digit decimal, in $\frac{1}{10}$ °C or °F 88880 = temperature-overflow 75550 = exceed max. sensor head temp. 74440 = fall below min. sensor head temp. 02563 = 256.3 °C or °F; -0170 = -17.0 °C or °F
repeatedly reading measuring values:	AAmsXXX	XXX = 000 ... 999 XXX = Number of measuring values
Emissivity:	AAemXXXX	XXXX = 0100 ... 1200 in ‰
Response time t_{90} :	AAezX	X = 0 ... 6 (decimal) 0 = intrinsic time constant of the device 1 = 0.5 s 2 = 1 s 3 = 2 s 4 = 5 s 5 = 10 s 6 = 30 s
Setting clear time t_{cl} :	AAIzX	X = 0 ... 8 (decimal) 0 = Max. value- / min. value storage off 1 = 0.10 s 5 = 5.00 s 2 = 0.25 s 6 = 25.00 s 3 = 0.50 s 7 = external clearing 4 = 1.00 s 8 = automatic clearing
External clearing:	AAIx	Simulation of an external reset contact
Setting maximum / minimum value:	AAmiX	X = desired setting 0 = maximum value, 1 = minimum value
Read. max/min value:	AAmi	Output: 0 or 1; 0 = max value, 1 = min value
Reading basic measuring range:	AAmb	Output: YYYYYZZZ (8-digit hex) ²⁾ YYYY = beginning of measuring range ZZZZ = end of measuring range
Reading sub range:	AAme	as with mb
Setting sub range:	AAm1YYYYZZZZ	YYYY = beginning of measuring range ZZZZ = end of measuring range
Analog output ¹⁾ :	AAasX	X = 0 ... 4 2 = 0 ... 5 V 0 = 0 ... 20 mA 3 = thermocouple type K 1 = 4 ... 20 mA 4 = thermocouple type J
Temperature display ¹⁾ :	AAfhX	X = 0;1 0 = Output Celsius 1 = Output Fahrenheit
Reading ambient temperature:	AAut	Output: stored value, 4-digit hex ²⁾ e.g. 0258 corresponds to 600 degrees
Entering ambient temperature:	AAutXXXX	XXXX = Value of ambient temp., 4-digit hex ²⁾ XXXX z.B. FFEC corresponds to -20 degrees -99 _{dez} = FF9D _{hex} means: automatic, no manual compensation
Sensor head temp.:	AAgt	Output: XXX (dec. 000...180 °C or 032...356 °F)
Max. sensor head temp.:	AAtm	Output: XXX (dec. 000...180 °C or 032...356 °F)
Baud rate:	AAbrX	X = 0 ... 4 0: 1200 bd 1: 2400 bd 2: 4800 bd 3: 9600 bd 4: 19200 bd
Instrument address ¹⁾ :	AAgaXX	XX: device address decimal; 00 ... 31 variable device addresses; global: 98, 99
Reading switch point:	AAsl	Output: XXXX (4-digit hex) ²⁾
Setting switch point:	AAslXXXX	XXXX (4-digit hex) ²⁾ ; adjustable within sub range

Reading hysteresis:	AAhIXX	XX (2-digit hex) ²⁾ ; XX setting 2 ... 20°C (4 ... 36°F)
Setting hysteresis:	AAhl	Output: XX (2-digit hex) ²⁾
Wait time:	AAtwXX	XX = 00 ... 99 relative delay value
Reading sensor data:	AAse	Output: XXXXYYYY (8-digit decimal); Reading of adjusted sensor data: XXXX: S1; YYYY: S2
Setting sensor data:	AAseXXXXYYYY	XXXXYYYY (8-digit dec.); entering sensor data
Reset ¹⁾ :	AAre	Reset device
Reading parameters:	AApa	Output 11-digit decimal: Digit 1 and 2 (10...99 or 00): EMI up to 100 Digit 3 (0 ... 6): t_{90} (response time) Digit 4 (0 ... 8): t_{cl} (storage clear mode) Digit 5 (0 / 4): analog output Digit 6 and 7 (00 ... 99): sensor head temp. Digit 8 and 9 (00 ... 31): device address Digit 10 (0 ... 4): device baud rate Digit 11 (always 0)
Error status:	AAfs	Output: XX; XX=00...FF (00 = no error) (01...FF: error code for LumaSense service)
Serial number:	AAsn	Output: XXXXX (5-digit decimal)
Type / software version:	AAve	Output: XYZZZ (6-digit decimal) XX = 76 (IN 510, IN 520, IN 530); YY = Month of software version ZZ = Year of software version

Notes: The letter "l" means the lower case letter of "L"

Bold values = default settings

- After entering these commands the device carries out an automatic reset. The device needs approx. 150 ms before it is ready to use and work with the changed settings.
- The input and output corresponds to the preset degree C or degree F.

Additional instruction for the RS485 interface

Requirements to the master system during half-duplex operation:

1. After an inquiry, the bus should be switched into a transmission time of 3 bits (some older interfaces are not fast enough for this).
2. The pyrometer's response will follow after 5 ms at the latest.
3. If there is no response, there is a parity or syntax error and the inquiry has to be repeated.

After receiving the response, the master has to wait at least 1.5 ms before a new command can be entered.

8 Reference numbers

8.1 Reference numbers instruments

3 874 360	IN 510	with sensor head 2:1	(85 °C ambient temperature),	3 m cable
3 874 370	IN 510	with sensor head 2:1	(85 °C ambient temperature),	15 m cable
3 874 460	IN 510	with sensor head 10:1	(85 °C ambient temperature),	3 m cable
3 874 470	IN 510	with sensor head 10:1	(85 °C ambient temperature),	15 m cable
3 874 160	IN 510-N	with sensor head 2:1	(85 °C ambient temperature),	3 m cable
3 874 170	IN 510-N	with sensor head 2:1	(85 °C ambient temperature),	15 m cable
3 874 260	IN 510-N	with sensor head 10:1	(85 °C ambient temperature),	3 m cable
3 874 270	IN 510-N	with sensor head 10:1	(85 °C ambient temperature),	15 m cable
3 874 380	IN 520	with sensor head 2:1	(180 °C ambient temperature),	3 m cable
3 874 390	IN 520	with sensor head 2:1	(180 °C ambient temperature),	15 m cable
3 874 480	IN 520	with sensor head 10:1	(180 °C ambient temperature),	3 m cable
3 874 490	IN 520	with sensor head 10:1	(180 °C ambient temperature),	15 m cable
3 874 180	IN 520-N	with sensor head 2:1	(180 °C ambient temperature),	3 m cable
3 874 190	IN 520-N	with sensor head 2:1	(180 °C ambient temperature),	15 m cable
3 874 280	IN 520-N	with sensor head 10:1	(180 °C ambient temperature),	3 m cable
3 874 290	IN 520-N	with sensor head 10:1	(180 °C ambient temperature),	15 m cable

8.2 Reference numbers accessories

3 821 010	Connection cable 2 m, 10 wire, with additional digital cable (1 m) and <i>InfraWin</i> analyzing and reporting software
3 821 020	Connection cable 2 m, for power supply and thermocouple output (compensating cable)
3 874 830	Sensor head 2:1 for IN 510, sensor cable 3m
3 874 840	Sensor head 2:1 for IN 510, sensor cable 15m
3 874 860	Sensor head 10:1 for IN 510, sensor cable 3m
3 874 870	Sensor head 10:1 for IN 510, sensor cable 15m
3 874 780	Sensor head 2:1 for IN 520, sensor cable 3m
3 874 790	Sensor head 2:1 for IN 520, sensor cable 15m
3 874 880	Sensor head 10:1 for IN 520, sensor cable 3m
3 874 890	Sensor head 10:1 for IN 520, sensor cable 15m

- 3 848 790 Close focus lens (only for 10:1 optics, max. 85 °C ambient temperature, not in combination with air purge, cooling / purging unit or 90° mirror)
- 3 834 380 Adjustable mounting angle (for sensor head or air purge with sensor head 10:1)
- 3 835 330 Air purge (for sensor head 10:1)
- 3 835 410 Air purge (for sensor head 2:1)
- 3 834 260 Adjustable mounting angle (for air purge with sensor head 2:1)
- 3 835 340 90° mirror (sensor head 10:1)
- 3 852 290 DIN-rail-power supply NG DC; 100 ... 240 V AC, 50 ... 60 Hz ⇒ 24 V DC, 1 A
- 3 890 560 DA 6000-N: LED-digital display with possibility for pyrometer parameter setting; RS232 interface
- 3 890 570 DA 6000-N with RS485 interface
- 3 826 500 HT 6000: portable indicator and instrument for pyrometer parameter setting
- 3 852 440 IMPAC Protocol converter RS485 ⇔ Profibus-DP (max. 1 instrument)
- 3 852 460 IMPAC Protocol converter RS485 ⇔ Profibus-DP (max. 32 instruments)

LumaSense Technologies

Temperature and Gas Sensing Solutions

上海麦兴仪器设备有限公司
Shanghai MaxSun Industrial Co., Ltd.

地址：上海市浦东新区张杨路188号汤臣中心A座
邮编：200122
电话：(86 21) 5888 6718 / 133 8186 8102
传真：(86 21) 5888 7876
邮箱：mx@imaxsun.com

麦兴（中国）有限公司
MaxSun (China) Limited.

地址：香港湾仔告士打道151号国卫中心11楼
电话：(852) 2836 8361
传真：(852) 3011 5863
邮箱：mx@imaxsun.com